



BIOPTIC 200

Liquid finishing product for ultrasonic or spray cleaning.

COMPATIBILITY:

- Titanium
- Stainless steel
- Nitinol
- Ceramics, plastics

INGREDIENTS:

- Organic acid
- Surfactants

PHYSICAL AND CHEMICAL DATA:

- concentrated pH: 0.9
- pH (1%): 2.3
- Density: 1.215
- Surface tension: 40.2 mN/m


INSTRUCTIONS FOR USE:

Optimum use conditions may be affected by the quality of the water used in the baths, as well as the type and quantity of contaminants.


- Concentration: 0.5 to 2%
- Temperature: 40 to 65°C (104 to 149°F)
- Time: 1-5 minutes

PROCESS EXAMPLES:

- Medical (dental) line / Spraying range

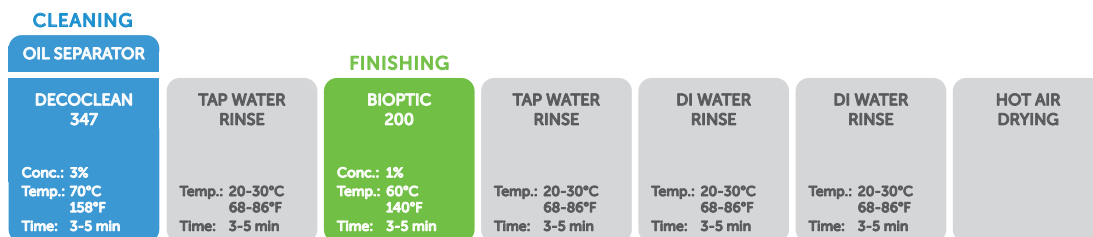

- Cleaning of watch sapphires (final cleaning) / Ultrasonic range

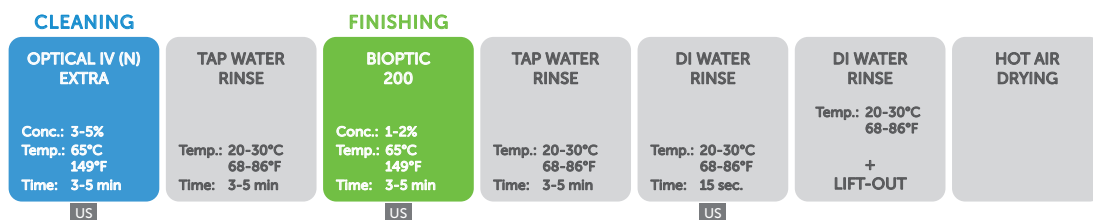

BENEFITS:

- Perfect dispersion and solubilization of contamination
- Very high finishing degree
- Exceptional longevity of the baths
- Spot-free surfaces after drying

STORAGE CONDITIONS:

- Keep the recipient hermetically sealed between 5°C and 40°C (41°F and 104°F) in a dry place.
- Always keep in packaging made from the same material as the original packaging.

23/02/21



If you have any questions, please contact our Application Centre on: +41 22 365 46 66

